

Test Requirement:

According to the requirement of the Module C2 (SPC CE-062_EN M5 PPE) of Applus+, the test item(s) of the sample is according to the standard EN149:2001+A1:2009.

Product Name: Filtering half mask

Report No.: PTC21022001102C-EN01

APPLUS +With ID

number:

21/32302544

Client: IVROU NETHERLANDS B.V.

Client Address: Lutkemeerweg 298, 1067 TH Amsterdam Netherlands

Manufacturer: Guangzhou Carrot Mall Network Technologies Co., Ltd.

Manufacturer Address: Room 1406, No.4 Zhudian Road (Nansha Street), Nansha District,

Guangzhou, Guangdong Province, China

Contact:

Model(s):

IRYS-02

Classification: Dedicated to Health

Date of Tests: 2021.05.21~2021.05.27

Signed for and on Behalf of PTC

Prepare by: Checked by:

This report is issued according to the general clauses in www.ptc-testing.com by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.

The report could not be copied without permission

IFICATION

Approved by:



Summary of assessment

Clause	Assessment
7.3 Visual inspection	PASS
7.5 Material	PASS
7.9.1 Total inward leakage	PASS
7.9.2 Penetration of filter material	PASS
7.12 Carbon dioxide content of the inhalation air	PASS
7.16 Breathing resistance	PASS
7.18 Demountable parts	PASS

Remark:

PASS: comply with requirement of standard



Dedicated to Health



Test Result:

Test Result	Conclusion
Comply	Pass

7.5 Material

Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used.

Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer.

After undergoing the conditioning described in 8.3.1 none of the particle filtering half masks shall have suffered mechanical failure of the facepiece or straps.

No mechanical failure after undergoing the conditioning described in 8.3.1,

Pass

No collapse when conditioned in accordance with 8.3.1 and 8.3.2.

When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse.

7.9.1 Total inward leakage

For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than 25 % for FFP1, 11 % for FFP2, 5 % for FFP3 and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than 22 % for FFP1, 8 % for FFP2, 2 % for FFP3.

FFP2, Test results are shown in Annex A Table 7.9.1-A&B

Pas:

7.9.2 Penetration of filter material

The penetration of the filter of the particle filtering half mask shall meet the requirements of Table 1.

	Sodium chloride test 95 l/min	Paraffin oil test 95 l/min
FFP1	≤ 20%	≤ 20%
FFP2	≤ 6%	≤ 6%
FFP3	≤ 1%	≤ 1%

FFP2, Test results are shown in Annex A Table 7.9.2.

Pass



7.12 Carbon dioxide content of the inhalation air

The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume)

Test results are shown in Annex A Table 7.12.

Pass

7.16 Breathing resistance

	Maximun	num permitted resistance (mbar)					
Classification	Inhal	Exhalation					
	30 l/min	95 l/min	160 l/min				
FFP1	0.6	2.1	3.0				
FFP2	0.7	2.4	3.0				
FFP3	1.0	3.0	3.0				

FFP2. Test results are shown in Annex A Table 7.16.

Pass

7.18 Demountable parts

All demountable parts (if fitted) shall be readily connected and secured, where possible by hand

Comply

Pass

SIGMAMEDICAL

Dedicated to Health



Annex A: Summarization of Test Data

Table 7.9.1-A: Inward Leakage Test Data

Test specification: EN 149:2001+A1:2009 Clause 8.5

Subject	Sample No.	Condition	Walk (%)	Head Side/side (%)	Head up/down (%)	Talk (%)	Walk (%)	Mean (%)
Lv	1	A.R	3.4	3.7	3.4	4.1	3.7	3.7
Li	2	A.R	4.5	4.8	4.6	4.6	4.5	4.6
Zhong	3	A.R	4.0	4.2	4.1	4.5	4.1	4.2
Xu	4	A.R	3.8	3.9	3.9	4.2	3.8	3.9
Ma	5	A.R	3.4	3.6	3.7	3.9	3.6	3.6
Chen	6	T.C	4.0	4.9	4.9	4.7	4.7	4.6
Chen	7	T.C	3.7	4.2	4.2	4.3	4.1	4.1
Zhuo	8	T.C	4.1	4.5	4.7	5.0	5.0	4.7
Chen	9	T.C	3.8	4.1	3.9	4.2	3.8	4.0
Zhang	10	T.C	3.5	3.5	3.7	3 .8 ■	3.2	3.5

Face Width Face Length Face Depth Mouth Width Subject 139 G04 LT Lv 53 Li 120 135 112 55 135 Zhong 108 106 56 Xu 120 150 120 70 Ma 130 170 130 Chen 110 160 90 40 Chen 115 145 110 50 Zhuo 103 146 100 50 95 40 Chen 110 145 Zhang 144 141 101 54



Table 7.9.2: Penetration of filter material

Test specification: EN 149:2001+A1:2009 Clause 8.11

Aerosol	Condition	Sample No.	Penetration (%)	Assessment
Sec. 16. 16. 15	h - 4. 4. 4. 4. 4.	11	0.7	4. 4. 8
10 miles - 10 miles	As received	12	0.6	S. 18 A. 18 A.
A STATE OF THE STA		13	0.6	Mary Mary
		14	0.2	30° 30° 3
Sodium chloride test	Simulated wearing treatment	15	0.5	
March St. March	The state of the state of	16	0.4	20 40 4
Paraffin oil test		17	0.3	1 100 100 11
	Mechanical strength + Temperature conditioned	18	0.4	
	remperature conditioned	19	0.4	Pass
	2001 (0001 2001 1005 2001	20	0.3	Pass
	As received	21	0.2	S. S. &
		22	0.3	1.30 .å .i
	MAN	23	0.2 ^	3. 8. 8
	Simulated wearing treatment	24	0.2	10 AC 10
	D 11.2	25	0.3	
	Dedicate	d to He	ealth	
- 40° - 40°	Mechanical strength + Temperature conditioned	27	0.8	43 40 .
the fact of the	remperature contantoried	28	0.8	6, 6, 4

Table 7.12: Carbon dioxide content of the inhalation air

Test specification: EN 149:2001+A1:2009 Clause 8.7

Condition	Sample No.	Re	Result (%)			
	29	0.04		a to the t		
As received	30	0.04	Mean value:	Pass		
	31	0.05	0.04			



Table 7.16: Breathing resistance (mbar)

Test specification: EN 149:2001+A1:2009 Clause 8.9

67-61	Flow Ra	ite	-9		32			+ T		33			4		34		
	30 I/min	Ja . 12	U .	0.32	,ĠL	eb i	26		0.31	- 24	1.1		ď	0.34	den.	jo	
As received	Inhalation	95 I/min			1.16					1.18					1.18		§ 20
	Exhalation	160	Α	В	С	D	Е	Α	В	С	D	Е	А	В	С	D	Е
36 36 B	Landidion	I/min	1.83	1.84	1.82	1.82	1.83	1.78	1.78	1.76	1.77	1.76	1.74	1.77	1.76	1.76	1.75
	Flow Ra	ite			35					36					37		
Simulated wearing Inhalation I/m	30 I/min			0.29					0.29					0.29			
	95 I/min	1.13			1.13				1.08								
Evhalation	Exhalation	160	Α	В	С	D	E	А	В	С	D	E	А	В	С	D	E
	l/min	1.69	1.69	1.68	1.66	1.68	1.66	1.66	1.66	1.64	1.65	1.64	1.66	1.65	1.64	1.65	
	Flow Ra	ite			38					39					40		
Temperature	Inhalation	30 I/min			0.35		41			0.31				IJ.,	0.33	ĮĠ.	, Ó
Temperature Inhalation conditioned	95 I/min		7	1.22	P	41			1.21				8	1.17			
	Exhalation	160	А	В	С	D	Е	А	В	С	D	E	А	В	С	D	Е
	EXIIdiduOII	I/min_	1.82	1.81	1.82	-1.78	1.78	175	1.72	172	1 73	1.71	1.86	1.82	1.85	1.83	1.84
Assessment				UII	Ca	CC		Pa		ai	CII		THE	1			

A: Facing directly ahead B: Facing vertically upwards C: Facing vertically downwards




Test	Uncertainty
Total inward leakage	3.8%
Penetration of filter material(NaCl)	3.5%
Penetration of filter material(Paraffin oil)	4.2%
Carbon dioxide content of the inhalation air	4.5%
Breathing resistance(30L/min)	5.2%
Breathing resistance(95L/min)	5.4%
Breathing resistance(160)L/min)	6.0%

Photo(s) of Sample:





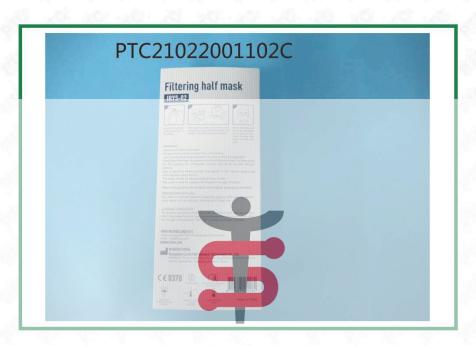













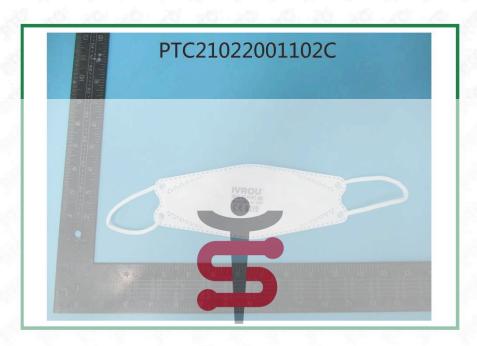






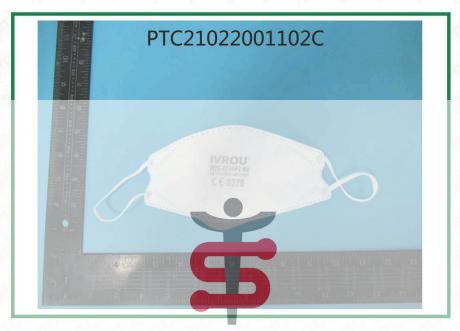





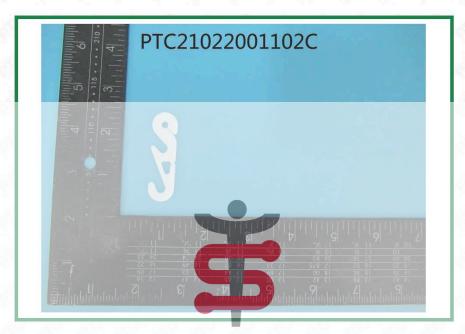

End of Report

SIGMAMEDICAL

Dedicated to Health